1/3


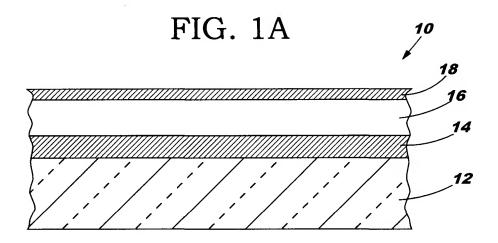


FIG. 1B

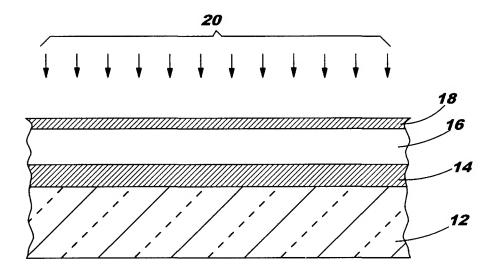

2/3

FIG. 1C


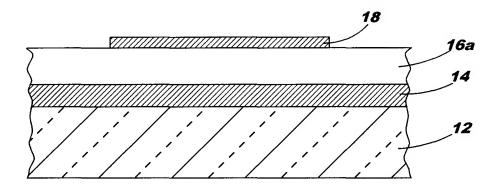


FIG. 1B

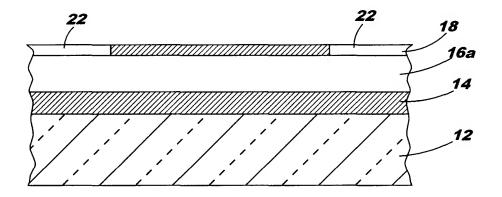

3/3 FIG. 2


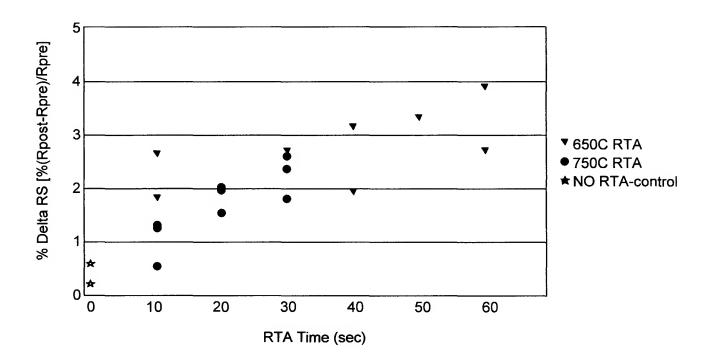


FIG. 3

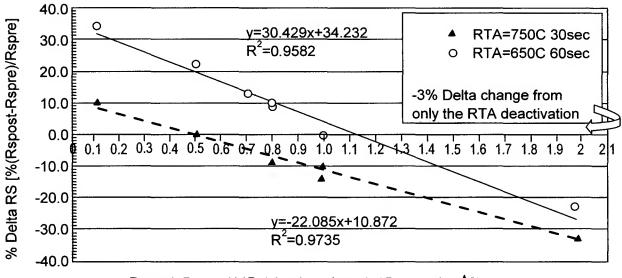

Rework Boron (11B+) Implant dose (e15 atoms/cm<sup>^2</sup>)

Page	24	of	24
------	----	----	----